RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

DrägerService®

Dräger

Field Service Procedure

Part Number: SP00215
Rev: -
Date: 20 Jume 2001
© 2001 Draeger Medical, Inc.

Saturn WPU Cable Guard Installation

RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

Saturn WPU
Cable Guard Installation

Installation Procedure

1. Position the cable guard on the Saturn WPU as shown in Figure 1. Orient the guard so that its mounting holes line up with those in the WPU.

NOTE: Additional holes are provided in the guard to accommodate several models of the WPU with different hole locations. Be sure to choose the correct mounting holes for your installation.

2. Secure the guard with the four #6 x ½ pan hd self-tapping screws provided in the kit.

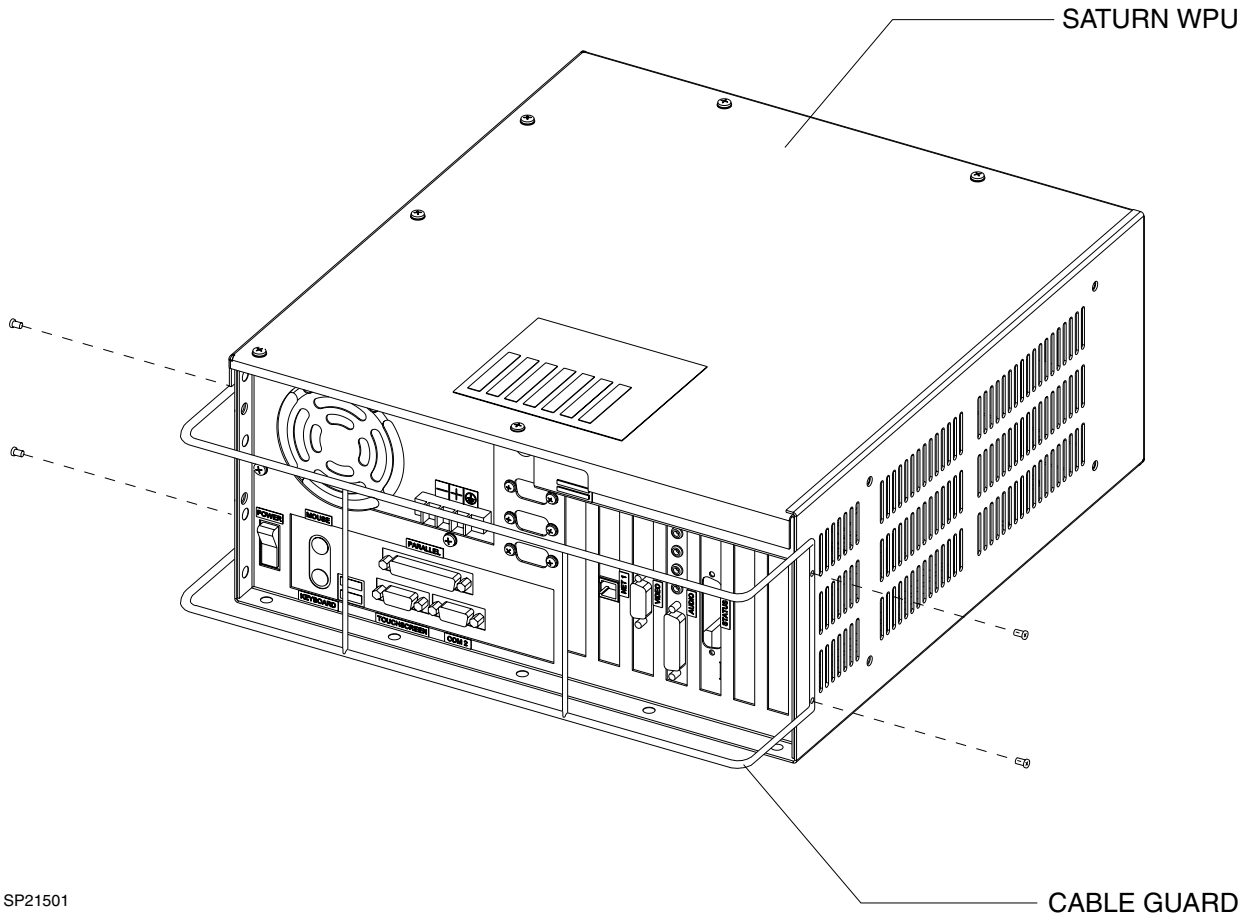

FIGURE 1. WPU Cable Guard Installation

RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

DrägerService®

Dräger

DrägerService is a division of
Draeger Medical, Inc.
3122 Commerce Drive
Telford, PA 18969
Tel: (215) 721-5402
(800) 543-5047
Fax: (215) 721-5784
Web: www.draegermedical.com
Printed in the U.S.A.